

Fast Fit[®] Sizing Jig | Printable Version Left Foot – Top





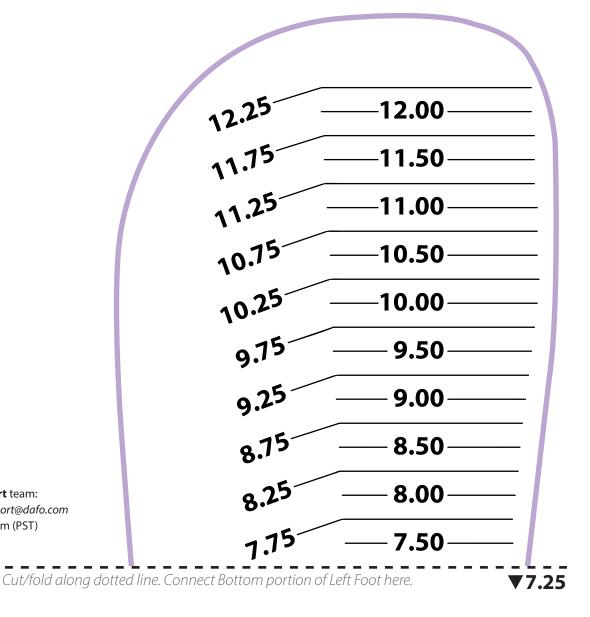

Questions?

Contact our **Customer Support** team: 800.848.7332 | *customersupport@dafo.com* Monday–Friday, 6:00am–5:00pm (PST)

To ensure accurate scaling and proper sizing,

1. With the Printable Sizing Jig pdf open in

5. After printing, verify that the scale on this

sheet is accurate with a standard ruler.

Adobe Reader, go to the File menu.

use the following printer settings:

2. Click the Print sub-menu item.

3. Make sure scale is set at 100%.

Print

4. Print.

Assemble

- 1. Follow the printing instructions (to the left). If the scaling is accurate, continue on.
- 2. Cut/fold along the dotted lines on the jigs' Top and Bottom portions.
- 3. Tape the Top and Bottom portions of the Left and Right sizing jigs at their corresponding dotted lines.

Size


 Make sure the patient is wearing socks and have him/her stand on the jig. Align the outermost part of the heel and the inside of the foot with the designated lines on the jig.

*See Figures 1 and 2 above.

- 2. Choose the length that will allow ¼ to ½ inch (.64 to 1.3 cm.) for growth.
- 3. Unless the patient's foot is significantly narrow, we recommend ordering a Wide size.

Printable Sizing Jig-outline — Left Top rev.04 (March 2024)

Fast Fit[®] Sizing Jig | Printable Version Left Foot – Bottom

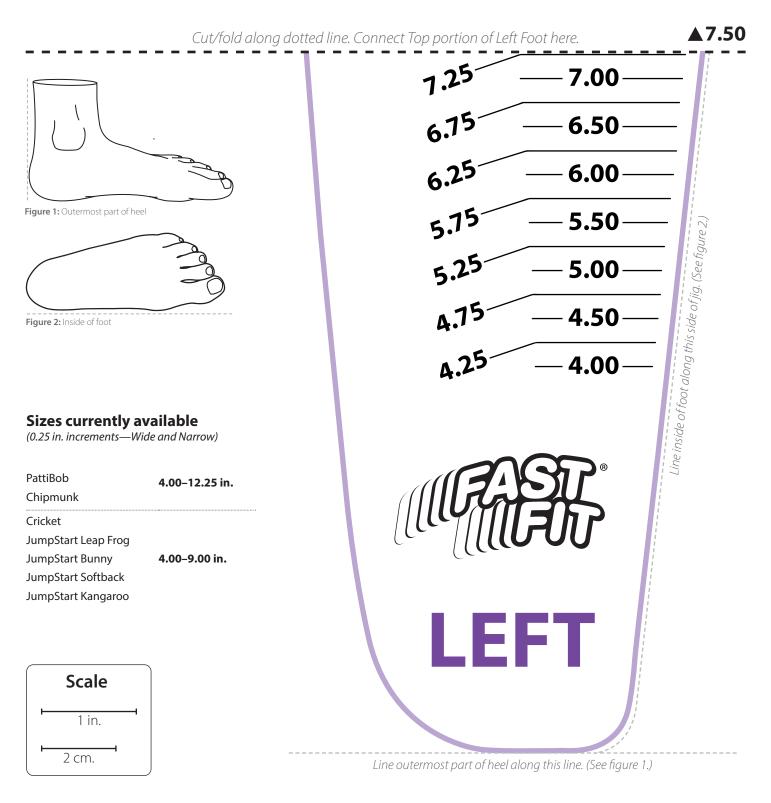



Printable Sizing Jig-outline — Left Bottom rev.04 (March 2024)

1360 Sunset Avenue Ferndale, WA 98248 ph: 800.848.7332 fax: 855.543.0092

Fast Fit[®] Sizing Jig | Printable Version Right Foot – Top





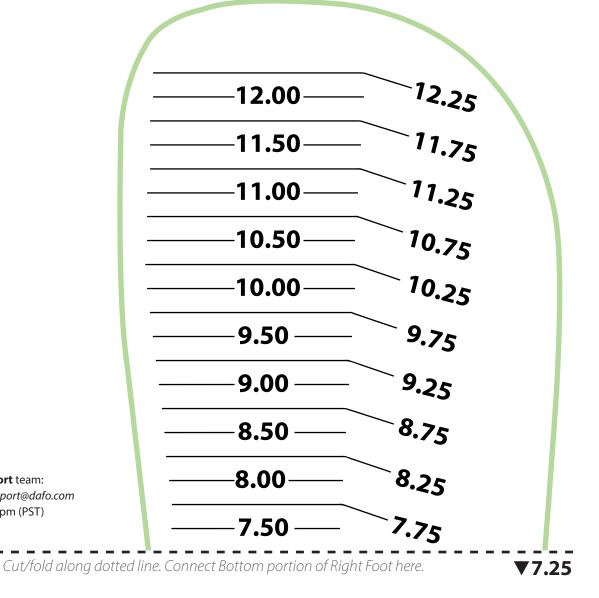

Questions?

Contact our **Customer Support** team: 800.848.7332 | *customersupport@dafo.com* Monday–Friday, 6:00am–5:00pm (PST)

Print

To ensure accurate scaling and proper sizing, use the following printer settings:

- 1. With the Printable Sizing Jig pdf open in Adobe Reader, go to the File menu.
- 2. Click the Print sub-menu item.
- 3. Make sure scale is set at 100%.
- 4. Print.
- 5. After printing, verify that the scale on this sheet is accurate with a standard ruler.

Assemble

- 1. Follow the printing instructions (to the left). If the scaling is accurate, continue on.
- 2. Cut/fold along the dotted lines on the jigs' Top and Bottom portions.
- 3. Tape the Top and Bottom portions of the Left and Right sizing jigs at their corresponding dotted lines.

🕄 Size

 Make sure the patient is wearing socks and have him/her stand on the jig. Align the outermost part of the heel and the inside of the foot with the designated lines on the jig.

*See Figures 1 and 2 above.

- 2. Choose the length that will allow ¼ to ½ inch (.64 to 1.3 cm.) for growth.
- 3. Unless the patient's foot is significantly narrow, we recommend ordering a Wide size.

Fast Fit[®] Sizing Jig | Printable Version Right Foot – Bottom



Printable Sizing Jig-outline — Right Bottom rev.04 (March 2024)

1360 Sunset Avenue Ferndale, WA 98248 ph: 800.848.7332 fax: 855.543.0092